




Return electrodes

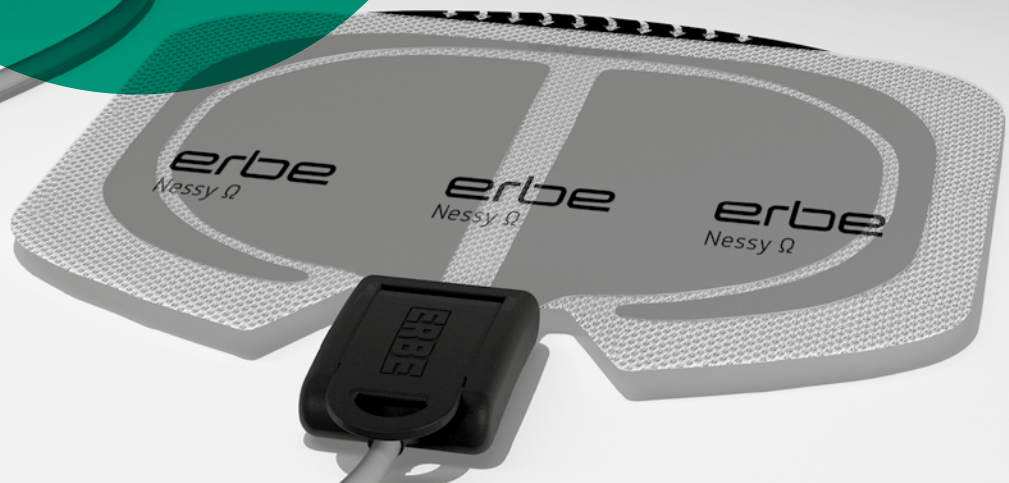

Legend

Important notes








The authors and Erbe Elektromedizin GmbH have taken the greatest possible care while compiling the catalogue with electrosurgical accessories. Nevertheless, it is impossible to exclude the possibility that errors may be contained herein.

The information and recommendations given here may not be construed as constituting any basis for any claims against Erbe Elektromedizin GmbH. Should legal regulations stipulate liability, such liability shall be limited to intentional misconduct or gross negligence.

The data on the use of instruments is based on clinical experience. Medical science is subject to a process of permanent change based on research and clinical experience. Therefore the products are subject to alterations in design and technique. Because of production tolerances dimensions in the catalogue may marginally differ.

We confirm that none of our products contain latex, except the rubber straps, Art. No. 20592-009 and 20592-011.

Further product information

Packaging unit	 = 5	 4 kVp	Max. electrical capacity
Notes on use	 30191-682	 max 95 °C	Temperature for cleaning in washer disinfectors
		 max 134 °C	Temperature for sterilization in autoclave
			Single-use product
		STERILE R	Sterile packaging
		STERILE R STERILE EO	
			Manual cleaning and disinfection

Please read carefully the corresponding notes on use before using any instrument.

Electrosurgery

Return electrodes

- 04 Single-use with contact stud
- 06 Single use with connecting cable
- 07 Reusable silicone plates

The NESSY guarantee is also available in your language.



NESSY®-Guarantee NeutralElectrodeSafetySystem

Positive experiences with safe and incident-free application of millions of Erbe NESSY® return electrodes enable us to give the following guarantee to users of Erbe NESSY® split return electrodes:

Erbe Elektromedizin GmbH hereby indemnifies all surgeons and surgical staff, who have been instructed by Erbe employees or by Erbe authorised persons, as well as their employers, and will pay compensation for any statutory liability claims which may arise as a result of electrosurgical burns under the Erbe NESSY® split return electrode, insofar as the claims are not covered by the liability insurance of the user concerned.

This guarantee is applicable for any surgical procedure in which a properly functioning electrosurgical generator (listed in the Appendix to the Declaration of Conformity of Erbe return electrodes) equipped with an intact monitoring system for split return electrodes is used.

This guarantee is only valid if Erbe NESSY® split return electrodes No. 20193-070, -071, -074, -075, -077, -078, -082, -083, -084, -085 are applied and, where necessary, only the appropriate reusable connecting cables No. 20194-026, -027, -046, -057, -058, -061, -063, -065, -072, -074, -077, -078, -080, -081, -083, -087, -201, -202, -205, -206 are used.

In addition to the aforementioned conditions, the regulations as stated in the instruction and service manuals regarding electrosurgical generators and their accessories must be strictly adhered to.

This guarantee only applies on condition that Erbe and the liability insurance provider are notified of such a damage event within the valid notification period for such a corresponding occurrence in the country involved and are given the opportunity to examine all relevant items pertaining to the submitted claims in detail.

This guarantee will remain valid as long as the Erbe NESSY® split return electrodes are used under the aforesaid conditions.

Erbe Elektromedizin GmbH


Dr. Jochen Queck, Vice President Marketing



NESSY®-GUARANTEE

Erbe Elektromedizin GmbH Waldhornstraße 17 72072 Tübingen Deutschland

Return electrodes

Single-use with contact stud

Erbe Nussy Ω, split, VIO, ICC, ACC, contact surface 85 cm²



equipotential ring 23 cm², without connecting cable


No. 20193-082

= 50

30193-082



Erbe NESSY Plate 170, split, VIO, ICC, ACC, contact surface 168 cm²



without connecting cable


No. 20193-070

= 50

30193-080



Erbe NESSY Plate 70, split, VIO, ICC, ACC, contact surface 72 cm²



without connecting cable, for children from 5 to 15 kg


No. 20193-071

= 50

30193-080



Erbe MONOPlate 140, single, VIO, ICC, ACC, T-Series, contact surface 136 cm²



without connecting cable

No. 20193-072

= 50


30193-080



Return electrodes

Single-use with contact stud


Erbe MONOPlate 40, single, VIO, ICC, ACC, T-Series, contact surface 40 cm²



without connecting cable, for children < 5kg

No. 20193-073

 = 50

 30193-080



Connecting cables for return electrodes	Length	Piece	No.
Return electrode cable, VIO, ICC, ACC, T-Series, Standard, for return electrodes with contact stud	4 m 5 m	1 1	20194-077 20194-078
Return electrode cable, VIO, ICC, ACC, non-Erbe units, International, for return electrodes with split contact surface and contact stud	4 m 5 m	1 1	20194-080 20194-087
Return electrode cable, VIO, ICC, ACC, non-Erbe units, International, for return electrodes with single contact surface and contact stud	4 m 5 m	1 1	20194-079 20194-086
Return electrode cable, Martin Standard, for return electrodes with contact stud	4 m	1	20194-081

Return electrodes

Single use with connecting cable

Erbe NESSY Ω , split, VIO, ICC, ACC, non-Erbe units, International



contact surface 85 cm², equiptential ring 23 cm²,
with connecting cable 4 m


No. 20193-083

= 50

30193-082



Erbe NESSY Plate 170, split, VIO, ICC, ACC, non-Erbe units, International



contact surface 168 cm², with connecting cable 3 m


No. 20193-074

= 50

30193-080



Erbe NESSY Plate 70, split, VIO, ICC, ACC, non-Erbe units, International



contact surface 72 cm², with connecting cable 3 m,
for children from 5 to 15 kg


No. 20193-075

= 50

30193-080



Erbe MONOPlate 140, single, VIO, ICC, ACC, non-Erbe units, International



contact surface 136 cm², with connecting cable 3 m

No. 20193-076

= 50

30193-080



Adapters for return electrodes

Return electrode adapter, VIO, ICC, ACC, T-Series, Standard (NE 6 mm)
for return electrode cable International (NE 2-Pin)



Piece

1

No.

20183-014

Return electrodes

Reusable silicone plates

Return electrode of conductive silicone, single, 295 x 175 mm, contact surface 500 cm²



with connecting cable 40 cm, ECG connection ø 4 mm,
with connecting cable 40 cm with 2 rubber fastening straps,
length 125 cm (contain latex), additional connecting cable necessary

No. 20193-008

= 1

30193-079



Return electrode of conductive silicone, single, 170 x 111 mm, contact surface 187 cm²



with connecting cable 40 cm, ECG connection ø 4 mm,
with connecting cable 40 cm with one rubber fastening strap,
length 55 cm (contain latex), additional connecting cable necessary

No. 20193-016

= 1

30193-079



Rubber strap, perforated, with 2 fastening studs, 550 x 60 mm



contains latex

No. 20592-009

= 1



Rubber strap, perforated, with 2 fastening studs, 1250 x 60 mm



contains latex

No. 20592-011

= 1



Fastening stud for rubber strap 20592-009, 20592-011



No. 40592-003

= 1



Connecting cables for return electrodes	Length	Piece	No.
Return electrode cable, VIO, ICC, ACC, T-Series, Standard, for silicone plates	4 m 5 m	1 1	20194-070 20194-088
Return electrode cable, VIO, ICC, ACC, International, for silicone plates	4 m 5 m	1 1	20194-075 20194-089
Return electrode cable, Martin Standard, for silicone plates	4 m	1	20194-076



Erbe Elektromedizin GmbH
Waldhoernlestrasse 17
72072 Tuebingen
Germany

Phone +49 7071 755-0
Fax +49 7071 755-179
info@erbe-med.com
erbe-med.com